

(19)



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11)

EP 0 666 084 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
07.04.2004 Bulletin 2004/15

(51) Int Cl.⁷: **A61M 5/20**, A61M 5/24

(21) Application number: **95200195.6**

(22) Date of filing: **27.01.1995**

(54) **Automatic self-injection device**

Vorrichtung zur automatischen Selbstinjektion

Dispositif pour auto-injection automatique

(84) Designated Contracting States:
DE ES FR GB IT

(30) Priority: **02.02.1994 US 191263**

(43) Date of publication of application:
09.08.1995 Bulletin 1995/32

(73) Proprietor: **Becton Dickinson and Company**
Franklin Lakes, New Jersey 07417-1880 (US)

(72) Inventors:
• **Bitdinger, Ralf V.**
F-38320 Herbeys (FR)
• **Grimard, Jean-Pierre**
F-38450 Vif (FR)

• **Sams, Bernard**
London N12 8EG (GB)
• **Solomon, Donald D.**
Warwick, New York 10990 (US)

(74) Representative: **Rambelli, Paolo et al**
c/o JACOBACCI & PERANI S.p.A.
Corso Regio Parco, 27
10152 Torino (IT)

(56) References cited:
EP-A- 0 409 365 **EP-A- 0 595 508**
FR-A- 1 014 881 **GB-A- 2 239 180**
US-A- 2 752 918 **US-A- 4 863 429**
US-A- 5 092 842

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The field of the invention relates to injection devices for automatically dispensing premeasured quantities of material, and drive assemblies therefor.

2. Brief Description of the Prior Art

[0002] Injection devices such as syringes are widely used in the medical and veterinary fields. They are ordinarily employed by trained personnel who are capable of selecting the appropriate medication and administering the required dosage.

[0003] Specialized injection devices have been designed for situations where trained personnel are not available to administer medication. Such devices are usable by persons such as diabetics who self-inject insulin, allergy sufferers who may require an emergency injection of anti-histamines or other medication, and other patients where self-injection is either more convenient or necessary.

[0004] U.S. Patent No. 2,752,918 discloses one type of automatically operated injection device. Upon firing an actuating mechanism of this device, a needle is caused to penetrate the skin, medicament is injected through the bore of the needle, and the needle is retracted. The device includes a first coil spring for causing the needle to be projected beyond a nose piece and a second coil spring which is compressed during this procedure. The second spring, upon release of a clutch mechanism, then automatically urges an ampoule and stem rearwardly, causing retraction of the needle.

[0005] U.S. Patent No. 5,137,516, corresponding to GB-A-2 239 180, discloses another type of automatically operated injection device. The user first presses the device against the skin in order to move an internal shaft and sleeve assembly. An actuating button is then depressed, causing a button arm to spread the arms of a retention clip. The separation of these arms releases the head of the pusher rod, which is then moved forwardly under the force of a main coil spring. The pusher rod first moves the entire syringe against the force of a syringe spring. Once the needle has penetrated the skin, the syringe plunger is depressed by the pusher rod, causing the syringe to empty. The main spring of the patented device may be recoiled upon reloading of a new syringe assembly. Such reloading is accomplished by a force applied by the syringe piston directly upon the pusher rod of the device.

[0006] A number of other approaches have been taken for providing automatic injection of various materials. U.S. Patent Nos. 3,797,489, 4,484,910, 4,902,279 and 5,114,404 provide further examples of this type of device.

SUMMARY OF THE INVENTION

[0007] The invention concerns an injection device

which is safe to use, reliable, and which minimizes the trauma associated with the self-administration of medicines and materials.

[0008] In accordance with a first embodiment of the invention, an injection device is provided which includes a housing, a syringe assembly slidably mounted to the housing, and a constant force spring for moving the syringe assembly with respect to the housing and towards the skin of a patient. By providing a substantially constant force upon the syringe assembly as it moves with respect to the housing, the relatively high impact of coil spring driven devices is avoided. The device is also more easily recoiled than devices employing coil springs as the constant force spring does not exert an increasing resistance during the reloading procedure. The constant force spring is preferably employed for driving the piston within the syringe assembly as well as the syringe assembly itself. This is preferably accomplished through the use of a rod and a driver releasably coupled to the rod. The driver causes the syringe assembly to move within the housing until it is decoupled from the rod. The rod then causes the injection of fluid.

[0009] In accordance with another embodiment of the invention, the mounting of the syringe assembly to the drive assembly of the device causes the reloading of the drive assembly. To accomplish this function, one end portion of the syringe assembly is provided with an abutment member which engages the drive rod of the drive assembly as it is mounted to the drive assembly. This causes the drive rod to be urged rearwardly against the force of the drive spring until it is retained in a loaded storage position. The abutment member is preferably positioned such that it may be rotated out of engagement with the drive rod, thereby allowing the drive rod to move through the end portion of the syringe assembly to drive the piston in the cartridge or barrel portion thereof. The drive rod preferably includes an elongated groove for receiving the abutment member as it slides through the end portion of the syringe assembly.

[0010] A drive assembly for driving a syringe assembly in the manner described above is also provided. The drive assembly includes a drive rod and a driver for urging a syringe piston and syringe assembly, respectively.

[0011] Other aspects of the invention which provide important functional advantages include a pushbutton which is drawn within the device at the end of the injection procedure, thereby providing end-of-dose indication. The ability of the pushbutton to release the drive assembly of the device is preferably limited by a sleeve which ordinarily covers the needle assembly. Displacement of the sleeve is necessary before the pushbutton can be moved sufficiently to commence the injection procedure. The sleeve is preferably coupled to the device such that it covers the needle assembly upon disengagement from the skin.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012]

Fig. 1 is a top perspective view of an injection device according to the invention;

Fig. 2 is a similar view thereof after removal of a cap therefrom;

Fig. 3 is a sectional view thereof showing the device in a storage position;

Fig. 4 is a similar view showing the removal of the cap of the device;

Fig. 5 is a similar view showing the exertion of a force F against the sleeve of the device;

Fig. 6 is a similar view showing the compression of the actuating button, thereby causing the drive spring to drive the syringe assembly;

Fig. 7 is a similar view showing the device upon completion of the injection process;

Fig. 8 is a similar view showing the device upon removal from the skin of a patient;

Fig. 9 is a similar view showing removal of the spent syringe assembly from the drive assembly of the device;

Fig. 10 is a similar view showing the initial step in mounting a new syringe assembly to the drive assembly;

Fig. 11 is a similar view showing the new syringe assembly partially within the housing of the drive assembly;

Fig. 12 is a side elevation view showing the initial step in mounting a new syringe to the drive assembly;

Fig. 13 is a side elevation view showing the final step in mounting a new syringe assembly to the drive assembly;

Fig. 14 is an enlarged front end view showing a plug and drive rod of the device in position to load a new syringe assembly;

Fig. 15 is a similar view showing the positions of the plug and drive rod after the syringe assembly has been rotated to a selected position;

Fig. 16 is a front end view of the drive rod;

Fig. 17 is a front end view of the plug;

Fig. 18 is a bottom perspective view of the device, and

Fig. 19 is an exploded, perspective view of the device.

DETAILED DESCRIPTION OF THE INVENTION

[0013] An injection device 10 is provided which is particularly adapted for the self-administration of medicines and other materials. Referring to Figs. 1 and 2, the device includes a drive assembly including an elongate housing 12 which may be easily handled by a user. One end of the housing is closed, while the opposite end is mounted to a collar 14. A cap 16 is mounted to one end

of a sleeve 28 in adjoining relation to the collar. The cap is not rotatable upon the sleeve, and is employed in conjunction with the collar for mounting a syringe assembly to the drive assembly. A plurality of elongate ribs 18 on the exterior surface of the cap are used during the mounting procedure, which is described in detail below.

[0014] Fig. 3 shows the injection device 10 in the storage position. Referring to Figs. 3 and 18, a syringe assembly 20 is provided in accordance with the preferred embodiment of the invention. A plug 24 mounted to one end of the syringe assembly, and a needle assembly 26 mounted to the opposite end thereof. A sleeve 28 encloses the syringe assembly. The syringe assembly includes a cartridge 30 or barrel and a piston 32 slidably positioned within the cartridge. The cap 16 is removably mounted to one end of the sleeve. An annular slot 34 is defined by a pair of concentric walls of the cap. The end portion of the sleeve 28 is positioned within the annular slot.

[0015] A rubber shield 36 is positioned within the cap, and protects the needle 38 of the syringe assembly. The shield is frictionally retained by the cap, and is removable with the cap when the device is to be employed. Rotation of the cap causes rotation of the syringe assembly 20 and sleeve 28 with respect to the drive assembly.

[0016] A coil spring 40 is provided for resiliently urging the sleeve 28 with respect to the cartridge 30. The cartridge includes a flange 42 which abuts against one end of the spring. The other end of the spring engages a radially inwardly extending wall of the sleeve. A portion 44 of the sleeve extends behind the plug 24, thereby preventing the sleeve and plug from being disconnected from the syringe assembly. The spring 40 causes the sleeve to extend over the needle in its rest position, as shown in Figs. 3 and 9.

[0017] The drive assembly 45 of the device is designed for repeated use. The drive assembly housing 12 is comprised of two sections 12A, 12B secured to each other by ultra-sonic welding or other suitable procedure. An elongate drive rod 46 is positioned within the housing. Guide rails 47 integral with the housing 12 maintain the orientation of the rod. The rod 46 includes an integral saddle 48 at one end thereof. The opposite end of the rod is smaller in dimension such that it fits within the plug 24 and cartridge 30. A ramp 50 is defined on one side of the rod near the saddle end thereof. The opposite side of the rod includes a plurality of notches 52. An elongate groove 54 extends from the end of the rod within the cartridge for a distance corresponding to at least the maximum length of travel of the piston 32 within the cartridge 30.

[0018] A constant force spring 56 is provided for urging the rod 46 in the direction of the piston 32. The wound end of the spring 56 is cradled within the saddle 48. The other end of the spring is secured to the housing 12. While a coil spring could be used to propel the rod, such a spring does not exert a substantially constant force upon the rod as it moves axially through the hous-

ing. In order to insure that a coil spring exerts sufficient force at the end of the stroke of the rod, it must be compressed more than is actually required at the beginning of the stroke. This results in a relatively high impact upon the syringe assembly by the driving mechanism, and ultimately upon the epidermis of the patient. Such a driving mechanism is also more likely to be very audible to the user, which may tend to upset the user.

[0019] The force exerted by the constant force spring 56 is sufficient to overcome the friction between the piston 32 and the cartridge 30 and between the needle 38 and the user's skin. When the rod 46 is pushed back to the start position after firing, the user needs to exert only a constant force upon the rod. If a coil spring was employed in the drive assembly, a steadily increasing force would be required to reload the device.

[0020] A driver 58 is releasably coupled to the rod 46. The driver includes a generally cylindrical body through which the rod 46 extends. A radially inwardly extending pawl 60 is positioned within one of the notches 52 and connects the driver to the rod. The pawl 60 extends from a deflectable spring arm 62 of the driver. One end 62A of the arm includes a radially outwardly extending projection 64. One end of the driver abuts against the plug 24.

[0021] A pushbutton 66 is provided for engaging both the driver 58 and the sleeve 28. The pushbutton accordingly functions as retaining means for retaining the rod/driver assembly and the constant force spring in the storage position shown in Fig. 3, as well as an actuating member for releasing the retaining means. Referring to Fig. 3, the pushbutton includes a first engagement member 66A which releasably engages the driver. (Alternatively, the rod could be releasably engaged). It further includes a second engagement member 66B which engages a projection 28A of the sleeve. The second engagement member prevents the sleeve from being removed from the drive assembly, and also prevents the pushbutton from being inadvertently actuated.

[0022] The pushbutton further includes a projection 66C which extends through an opening in the housing 12. The pushbutton and projection are maintained in the position shown in Fig. 3 by a coil spring 68 which urges the pushbutton towards the opening, as well as by the sleeve projection 28A. When the sleeve projection is displaced rearwardly, as shown in Fig. 5, the coil spring 68 alone maintains the position of the pushbutton.

[0023] The first engagement member 66A of the pushbutton may be moved out of engagement with the driver 58 upon manually urging the pushbutton against the force of the compression spring 68. Fig. 6 shows the device shortly after release of the driver/rod assembly. Upon further travel of the driver/rod assembly, as shown in Fig. 7,

the ramp 50 defined on one side of the rod 46 engages the first engagement member 66A, thereby drawing the pushbutton further inside the housing 12. This movement causes the release of the sleeve 28, which is urged

by the sleeve spring 40 into a position covering the tip of the needle 38 (Fig. 8).

[0024] As discussed above, the plug 24 is mounted to one end of the syringe assembly 20, and an end of the driver 58 engages the plug. The plug includes an opening 24A through which the rod 46 passes when an injection is made. The plug further includes an abutment in the form of a radially inwardly extending projection 24B, as shown in Figs. 3-9, 14, 15 and 17. The syringe assembly is rotatable between a first position, as shown in Figs. 14, where the projection 24B abuts an end surface 46A of the rod, and a second position (Figs. 3 and 15) where the projection 24B is opposite the groove 54 in the rod. The rod is accordingly able to pass through the plug when the syringe assembly is in the second rotational position. About forty degrees of rotation are required to move the syringe assembly between the first and second positions.

[0025] The plug 24 further includes a radially outwardly extending projection 24C which is located within an axial slot 28D in the sleeve. An axial projection 24D extends from the plug, and may be used for alignment purposes when a new syringe assembly is loaded.

[0026] The housing 12 includes means for engaging the projection 64 of the driver, thereby causing the arm 62 thereof to pivot about an integral hinge portion as shown in Fig. 6. This, in turn, causes the pawl 60 to be withdrawn from the notch 62. The engaging means include

a radially inwardly extending projection 70 having an arcuate surface which engages a corresponding arcuate surface on the projection 64.

[0027] The operation of the device will be described with reference to Figs. 3-11 and 13-15. Fig. 3 shows the device in its storage position. The cartridge 30 contains the material to be injected, and the piston 32 is located towards the rear end of the cartridge. The radially inwardly extending projection 24B of the plug 24 is located opposite the groove 54 in the rod 46. The driver 58 is coupled to the drive rod 46. The pushbutton 66 engages the driver 58, thereby preventing movement of the rod/driver assembly under the force of the constant force spring 56. The pushbutton cannot be depressed to release the rod/driver assembly as the sleeve projection 28A abuts the second engagement member 66B of the pushbutton.

[0028] As shown in Fig. 4, the cap 16 is removed by pulling it forwardly along the longitudinal axis of the device. The shield 36 is removed with the cap. The device otherwise remains unchanged from the position shown in Fig. 3.

[0029] The end of the sleeve 28 is pressed against the epidermis, thereby causing a force F to be exerted thereon as shown in Fig. 5. The sleeve moves rearwardly against the force of the sleeve spring 40 for several millimeters, at which time the rear portion 44 of the sleeve engages a stop 12C extending from the housing 12. This movement is sufficient to displace the sleeve

projection 28A a sufficient distance that it no longer interferes with the downward movement of the pushbutton 66.

[0030] The projection 66C of the pushbutton is pressed manually towards the housing as shown in Fig. 6. This causes displacement of the first engagement member 66A such that it no longer engages the driver 58. The driver 58 and rod 46 move as a unit under the constant force of the spring 56, causing the syringe assembly 20 (via the plug 24) to move forwardly, and the needle 38 thereof to penetrate the skin. As the rod remains coupled to the driver, the piston 32 does not move. Once the needle has sufficiently penetrated the skin and underlying tissue, the projection 64 on the driver 58 engages the projection 70 extending inwardly from the housing 12. This causes the pivotable arm 62 of the driver to rotate, and the pawl 60 to move out of the notch 52. The driver 58 and rod are decoupled at this point, which is just prior to the bottoming of the sleeve spring 40.

[0031] Referring now to Fig. 7, the rod 46 is urged forwardly as the rear end of the constant force spring 56 rotates within the saddle 48. The rod now moves with respect to the driver 58, urging the piston 32 forwardly as fluid is displaced from the cartridge 30. The rod advances through the plug 24 as the groove 54 is aligned with the plug projection 24B. Movement of the rod continues until the piston 32 engages the end wall of the cartridge 30. The ramp 50 of the rod 46 engages the first engagement member 66A of the pushbutton near the end of its stroke, drawing the pushbutton entirely within the housing. This provides a visual end of dose indication. The sleeve 28 is released once the second engagement member 66B is sufficiently displaced with respect to the sleeve projection 28A.

[0032] Upon completion of the injection procedure, the device 10 is withdrawn from the body. The sleeve 28 moves forwardly under the force of the sleeve spring to again cover the needle 38, as shown in Fig. 8, and is releasably locked in position by a pawl 14A. The pushbutton remains within the housing, and accordingly cannot be actuated until a new syringe assembly is installed.

[0033] The disposable portion of the device is disconnected from the reusable portion by grasping the sleeve 28 and pulling it in the axial direction. This causes the displacement of the pawl 14A extending radially inwardly from the collar, from a notch 28B within the sleeve. The cap 16 can be replaced before or after removal of the disposable portion of the device.

[0034] A new syringe assembly is installed by grasping the cap 16 and aligning a longitudinal rib 28C on the sleeve with a slot 14B in the collar. It can then be pushed into the housing until the cap 16 engages the collar 14. When aligned in this manner, the plug projection 24B is in opposing relation to the end surface 46A of the rod rather than the groove 54 within the rod. Insertion of the disposable portion of the device 10 accordingly causes

the rod 46 to be pushed back into the housing 12. The wound end of the constant force spring 56 rotates in the saddle as the spring unravels. The rim of the plug 24 pushes back the driver 58 during this procedure.

[0035] The disposable portion can be rotated about an arc of forty degrees once it is pushed as far back as possible. Because the driver is pushed back with the rod, the pushbutton 66 springs back into the position shown in Fig. 3 as it moves partially within the gap of the driver. The driver pawl 60 moves into one of the notches 52 in the rod. The particular notch to be engaged by the pawl is determined by the length of the plug 24. If the piston 32 is located closer to the needle end of the cartridge, the nose portion of the plug will be longer such that it adjoins, but does not contact, the piston.

[0036] It will be appreciated that various modifications can be made to the device for various purposes. While not preferred, a pair of springs could be used to drive the syringe assembly and piston, respectively. One or both springs could be constant force springs, preferably both. While it is also highly preferred that the drive assembly be rearmed upon insertion of the syringe assembly, this step could also be accomplished as a separate procedure. The use of a constant force spring facilitates the rearming procedure regardless of which approach is employed. Rearming may also be accomplished without directly engaging the drive rod. It is sufficient that the rod be driven back against the force of the drive spring, whether by direct engagement of the rod or via an intermediate structure.

[0037] Although illustrative embodiments of the present invention have been described herein with reference to the accompanying drawings, it is to be understood that the invention is not limited to those precise embodiments, and that various other changes and modifications may be effected therein by one skilled in the art without departing from the scope as defined by the appended claims.

Claims

1. An automatic injection device (10) comprising:

- a housing (12);
- a syringe assembly (20) slidably mounted to said housing (12), said syringe assembly (20) including a cartridge (30) and a piston (32) slidably mounted within said cartridge (30);
- means (46, 56, 58) for causing said syringe assembly (20) to slide with respect to said housing (12) from a storage position to a deployed position, and
- means (46, 56) for causing said piston (32) to slide within said cartridge (30) from a first position to a second position such that the contents of said cartridge (30) are expelled, character-

- ized by the fact that said means (46, 56, 58) for causing said syringe assembly to slide include a constant force spring (56) which provides a substantially constant force upon said syringe assembly (20) between said storage and deployed positions; means (66, 66A) being provided for releasably retaining said constant force spring (56) in a selected position.
2. A device as described in Claim 1, wherein said means (46, 56) for causing said piston (32) to slide within said cartridge (30) include a constant force spring (56).
 3. A device as described in Claim 1, including a sleeve (28) mounted to said housing (12), said sleeve (28) including a first end portion adapted to engage the skin of a patient, a spring (40) urging said sleeve (28) in the direction of said first end portion, said sleeve (28) being retractable with respect to said housing (12) against the force of said spring (40) when sufficient pressure is exerted against said first position.
 4. A device as described in Claim 3 including a manually operated actuating member (66C) for releasing said constant force spring retaining means (66, 66A).
 5. A device as described in Claim 4 including means (28A) for selectively preventing said actuating member (66C) from releasing said constant force spring retaining means (66, 66A), said means (28A) for selectively preventing being coupled to said sleeve (28).
 6. A device as described in Claim 1 including an elongate rod (46), a driver (58) releasably coupled to said elongate rod (46), means (64, 70) for decoupling said elongate rod (46) from said driver (58), said driver (58) being engageable with said syringe assembly (20) for moving said syringe assembly with respect to said housing (12), said elongate rod (46) being engageable with said piston (32) for moving said piston with respect to said cartridge (30), said constant force spring (56) urging said driver (58) and elongate rod (46) towards said syringe assembly (20) and piston (32), respectively.
 7. A device as described in Claim 6, wherein said elongate rod (46) includes at least one notch (52), said driver (58) includes a first projection (60) extending radially inwardly within said notch (52) and a second projection (64) extending radially outwardly, said means (64, 70) for decoupling including means (70) for moving said second projection (64) for causing said first projection (60) to be withdrawn from said notch (52).
 8. A device as described in Claim 6, including a manually operated actuating member (66C) extending at least partially from said housing (12) and said elongate rod (46) includes means (50) for drawing said actuating member (66C) within said housing (12).
 9. A device as described in Claim 1 including a sleeve (28) releasably mounted to said housing (12) and enclosing at least part of said syringe assembly (20).
 10. A device as described in Claim 9 including an elongate rod (46) slidably mounted within said housing (12) and engageable with said piston (32), said constant force spring (56) urging said elongate rod (46) towards said piston; and a plug (24) mounted to said cartridge (30), said plug (24) including an abutment (24B) engageable with said rod (46) when said plug (24) is in a first rotational position, said rod (46) being movable through said plug (24) when said plug is in a second rotational position.
 11. A device as described in Claim 6 including a plug (24) mounted to one end of said syringe assembly (20), said plug including an abutment (24B) adjoining an end surface of said elongate rod (46) when said cartridge (30) is in a first rotational position, said syringe assembly (20) being rotatable to a second rotational position wherein said abutment does not adjoin said end surface of said elongate rod (46), thereby allowing at least a portion of said elongate rod (46) to pass through said plug.
 12. An automatic injection device (10) according to Claim 1, comprising a rod (46) and a driver (58) releasably coupled to said rod (46), wherein said constant force spring (56) is adapted to urge said rod (46) along the longitudinal axis of said housing (12) such that said driver (58) urges said cartridge (30) and said rod (46) urges said piston (32) along the longitudinal axis, means (64, 70) being provided for automatically decoupling said driver (58) and said rod (46) as said rod moves along the longitudinal axis such that said rod (46) moves said piston (32) with respect to said cartridge (30) upon said driver (58) being decoupled from said rod.

Patentansprüche

1. Automatische Injektionsvorrichtung (f10), die umfasst:
 - ein Gehäuse (12);
 - eine Spritzenbaugruppe (20), die verschiebbar

- an dem Gehäuse (12) angebracht ist, wobei die Spritzenbaugruppe (20) einen Zylinder (30) und einen Kolben (32) enthält, der verschiebbar in dem Zylinder (30) angebracht ist; eine Einrichtung (46, 56, 58), die bewirkt, dass die Spritzenbaugruppe (20) in Bezug auf das Gehäuse (12) aus einer eingefahrenen Stellung in eine ausgefahrene Stellung gleitet, und eine Einrichtung (46, 56), die bewirkt, dass der Kolben (32) in dem Zylinder (30) aus einer ersten Stellung in eine zweite Stellung gleitet, so dass der Inhalt des Zylinders (30) ausgestoßen wird, **dadurch gekennzeichnet, dass** die Einrichtung (46, 56, 58), die bewirkt, dass die Spritzenbaugruppe (20) gleitet, eine Feder (56) mit gleichbleibender Federkraft enthält, die eine im wesentlichen gleichbleibende Kraft auf die Spritzenbaugruppe (20) zwischen der eingefahrenen und der ausgefahrenen Stellung ausübt; eine Einrichtung (66, 66A) zum lösbaren Feststellen der Feder (56) mit gleichbleibender Federkraft in einer ausgewählten Stellung vorhanden ist.
2. Vorrichtung nach Anspruch 1, wobei die Einrichtung (46, 56), die bewirkt, dass der Kolben (32) in dem Zylinder (30) gleitet, eine Feder (56) mit gleichbleibender Federkraft enthält.
 3. Vorrichtung nach Anspruch 1, die eine Hülse (28) enthält, die an dem Gehäuse (12) angebracht ist, wobei die Hülse (28) einen ersten Endabschnitt, der mit der Haut eines Patienten in Kontakt kommt, eine Feder (40) enthält, die die Hülse (28) in Richtung des ersten Endabschnitts drückt, wobei die Hülse (28) in Bezug auf das Gehäuse (12) gegen die Kraft der Feder (40) zurückgezogen werden kann, wenn ausreichender Druck auf den ersten Abschnitt ausgeübt wird.
 4. Vorrichtung nach Anspruch 3, die ein manuell betätigtes Betätigungselement (66C) zum Lösen der Feststelleinrichtung (66, 66A) für die Feder mit gleichbleibender Federkraft enthält.
 5. Vorrichtung nach Anspruch 4, die eine Einrichtung (28A) enthält, mit der wahlweise verhindert werden kann, dass das Betätigungselement (66C) die Feststelleinrichtung (66, 66A) für die Feder mit gleichbleibender Federkraft löst, wobei die Einrichtung (28A) zum wahlweisen Verhindern mit der Hülse (28) verbunden ist.
 6. Vorrichtung nach Anspruch 1, die eine längliche Stange (46), einen Mitnehmer (58), der lösbar mit der länglichen Stange (46) verbunden ist, eine Einrichtung (64, 70) zum Trennen der länglichen Stange (46) von dem Mitnehmer (58) enthält, wobei der Mitnehmer (58) mit der Spritzenbaugruppe (20) in Eingriff gebracht werden kann, um die Spritzenbaugruppe in Bezug auf das Gehäuse (12) zu bewegen, wobei die längliche Stange (46) mit dem Kolben (32) in Eingriff gebracht werden kann, um den Kolben in Bezug auf den Zylinder (30) zu bewegen, und die Feder (56) mit gleichbleibender Federkraft den Mitnehmer (58) sowie die längliche Stange (46) auf die Spritzenbaugruppe (20) bzw. den Kolben (32) zu drückt.
 7. Vorrichtung nach Anspruch 6, wobei die längliche Stange (46) wenigstens eine Einkerbung (52) enthält, der Mitnehmer (58) einen ersten Vorsprung (60) enthält, der sich radial nach innen in der Einkerbung (52) erstreckt, sowie einen zweiten Vorsprung (64) enthält, der sich radial nach außen erstreckt, und die Einrichtung (64, 70) zum Trennen eines Vorsprungs (64) enthält, die bewirkt, dass der erste Vorsprung (60) aus der Einkerbung (52) herausgezogen wird.
 8. Vorrichtung nach Anspruch 6, die ein manuell betätigtes Betätigungselement (66C) enthält, das sich wenigstens teilweise von dem Gehäuse (12) weg erstreckt, und wobei die längliche Stange (46) eine Einrichtung (50) zum Ziehen des Betätigungselementes (66C) in dem Gehäuse (12) enthält.
 9. Vorrichtung nach Anspruch 1, die eine Hülse (28) enthält, die lösbar an dem Gehäuse (12) angebracht ist und wenigstens einen Teil der Spritzenbaugruppe (20) umschließt.
 10. Vorrichtung nach Anspruch 9, die eine längliche Stange (46), die verschiebbar in dem Gehäuse (12) angebracht ist und mit dem Kolben (32) in Eingriff gebracht werden kann, wobei die Feder (56) mit gleichbleibender Federkraft die längliche Stange (46) auf den Kolben zu drückt; sowie einen Stopfen (24) enthält, der an dem Zylinder (30) angebracht ist, wobei der Stopfen (24) einen Anschlag (24B) enthält, der mit der Stange (46) in Eingriff gebracht werden kann, wenn sich der Stopfen (24) in einer ersten Drehstellung befindet, wobei die Stange (46) durch den Stopfen (24) hindurchbewegt werden kann, wenn sich der Stopfen in einer zweiten Drehstellung befindet.
 11. Vorrichtung nach Anspruch 6, die einen Stopfen (24) enthält, der an einem Ende der Spritzenbaugruppe (20) angebracht ist, wobei der Stopfen einen Anschlag (24B) enthält, der an eine Endfläche der länglichen Stange (46) angrenzt, wenn sich der Zylinder (30) in einer ersten Drehstellung befindet, die Spritzenbaugruppe (20) in eine zweite Drehstel-

lung gedreht werden kann, in der der Anschlag nicht an die Endfläche der länglichen Stange (46) angrenzt, so dass wenigstens ein Teil der länglichen Stange (46) durch den Stopfen hindurchtreten kann.

12. Automatische Injektionsvorrichtung (10) nach Anspruch 1, die eine Stange (46) und einen Mitnehmer (58) umfasst, der lösbar mit der Stange (46) verbunden ist; wobei die Feder (56) mit gleichbleibender Federkraft die Stange (46) entlang der Längsachse des Gehäuses (12) drückt, so dass der Mitnehmer (58) auf den Zylinder (30) drückt und die Stange (46) den Kolben (32) entlang der Längsachse drückt; eine Einrichtung (64, 70) vorhanden ist, die den Mitnehmer (58) und die Stange (46) automatisch trennt, wenn sich die Stange entlang der Längsachse bewegt, so dass die Stange (46) den Kolben (32) in Bezug auf den Zylinder (30) bewegt, wenn der Mitnehmer (58) von der Stange gelöst wird.

Revendications

1. Dispositif (10) d'injection automatique, comprenant :

un boîtier (12) ;
un ensemble (20) à seringue monté de manière coulissante sur ledit boîtier (12), ledit ensemble (20) à seringue incluant une cartouche (30) et un piston (32) monté de manière coulissante à l'intérieur de ladite cartouche (30) ;
un moyen (46, 56, 58) servant à faire coulisser ledit ensemble (20) à seringue par rapport audit boîtier (12) d'une position rangée à une position déployée, et
un moyen (46, 56) servant à faire coulisser ledit piston (32) à l'intérieur de ladite cartouche (30) d'une première position à une seconde position, de façon à expulser le contenu de ladite cartouche (30), **caractérisé en ce que** ledit moyen (46, 56, 58) servant à faire coulisser ledit ensemble à seringue comprend un ressort à force constante (56) qui applique une force sensiblement constante audit ensemble (20) à seringue entre lesdites positions rangée et déployée ;
un moyen (66, 66A) étant prévu pour maintenir de façon libérable ledit ressort à force constante (56) dans une position choisie.

2. Dispositif selon la revendication 1, dans lequel ledit moyen (46, 56) servant à faire coulisser ledit piston (32) à l'intérieur de ladite cartouche (30) comprend un ressort à force constante (56).

3. Dispositif selon la revendication 1, comprenant un manchon (28) monté sur ledit boîtier (12), ledit manchon (28) incluant une première partie d'extrémité apte à être engagée dans la peau d'un patient, un ressort (40) poussant ledit manchon (28) dans la direction de ladite première partie d'extrémité, ledit manchon (28) pouvant se rétracter par rapport audit boîtier (12) contre la force dudit ressort (40) lorsqu'une pression suffisante est exercée contre ladite première position.

4. Dispositif selon la revendication 3, comprenant un élément (66C) d'actionnement à fonctionnement manuel destiné à libérer ledit moyen (66, 66A) de maintien de ressort à force constante.

5. Dispositif selon la revendication 4, comprenant un moyen (28A) destiné à empêcher, sélectivement, que ledit élément (66C) d'actionnement ne libère ledit moyen (66, 66A) de maintien de ressort à force constante, ledit moyen (28A) assurant la fonction d'empêchement sélectif étant accouplé audit manchon (28).

6. Dispositif selon la revendication 1, comprenant une tige allongée (46), un dispositif d'entraînement (58) accouplé de manière libérable à ladite tige allongée (46), un moyen (64, 70) destiné à désaccoupler ladite tige allongée (46) dudit dispositif d'entraînement (58), ledit dispositif d'entraînement (58) pouvant engager ledit ensemble (20) à seringue pour déplacer ledit ensemble à seringue par rapport audit boîtier (12), ladite tige allongée (46) pouvant engager ledit piston (32) pour déplacer ledit piston par rapport à ladite cartouche (30), ledit ressort à force constante (56) poussant, respectivement, ledit dispositif d'entraînement (58) et ladite tige allongée (46) vers ledit ensemble (20) à seringue et ledit piston (32).

7. Dispositif selon la revendication 6, dans lequel ladite tige allongée (46) comprend au moins une encoche (52), ledit dispositif d'entraînement (58) comprend une première saillie (60) s'étendant radialement vers l'intérieur à l'intérieur de ladite encoche (52) et une seconde saillie (64) s'étendant radialement vers l'extérieur, ledit moyen (64, 70) de désaccouplement comprenant un moyen (70) servant à déplacer ladite seconde saillie (64) pour provoquer le retrait de ladite première saillie (60) de ladite encoche (52).

8. Dispositif selon la revendication 6, comprenant un élément (66C) d'actionnement à fonctionnement manuel s'étendant au moins partiellement dudit boîtier (12), et ladite tige allongée (46) comprend un moyen (50) destiné à tirer ledit élément (66C) d'actionnement à l'intérieur dudit boîtier (12).

9. Dispositif selon la revendication 1, comprenant un manchon (28) monté de manière libérable sur ledit boîtier (12) et confinant au moins une partie dudit ensemble (20) à seringue.

5

10. Dispositif selon la revendication 9, comprenant une tige allongée (46) montée de manière coulissante à l'intérieur dudit boîtier (12) et pouvant engager ledit piston (32), ledit ressort à force constante (56) poussant ladite tige allongée (46) vers ledit piston ;
et un raccord mâle (24) monté sur ladite cartouche (30), ledit raccord mâle (24) comprenant une butée (24B) pouvant engager ladite tige (46) lorsque ledit raccord mâle (24) se trouve dans une première position de rotation, ladite tige (46) étant mobile à travers ledit raccord mâle (24) lorsque ledit raccord mâle se trouve dans une seconde position de rotation.

10

15

11. Dispositif selon la revendication 6, comprenant un raccord mâle (24) monté sur une extrémité dudit ensemble (20) à seringue, ledit raccord mâle comprenant une butée (24B) contiguë à une surface d'extrémité de ladite tige allongée (46) lorsque ladite cartouche (30) se trouve dans une première position de rotation, ledit ensemble (20) à seringue pouvant tourner vers une seconde position de rotation lorsque ladite butée n'est pas contiguë à ladite surface d'extrémité de ladite tige allongée (46), en permettant ainsi qu'au moins une partie de ladite tige allongée (46) traverse ledit raccord mâle.

20

25

30

12. Dispositif (10) d'injection automatique selon la revendication 1, comprenant une tige (46) et un dispositif d'entraînement (58) accouplé de manière libérable à ladite tige (46), dans lequel ledit ressort à force constante (56) est apte à pousser ladite tige (46) le long de l'axe longitudinal dudit boîtier (12), de sorte que ledit dispositif d'entraînement (58) pousse ladite cartouche (30) et ladite tige (46) pousse ledit piston (32) le long de l'axe longitudinal, un moyen (64, 70) étant prévu pour désaccoupler automatiquement ledit dispositif d'entraînement (58) et ladite tige (46) lorsque ladite tige se déplace le long de l'axe longitudinal de façon que ladite tige (46) déplace ledit piston (32) par rapport à ladite cartouche (30) lors du désaccouplement dudit dispositif d'entraînement (58) et de ladite tige.


35


40



45



50

55

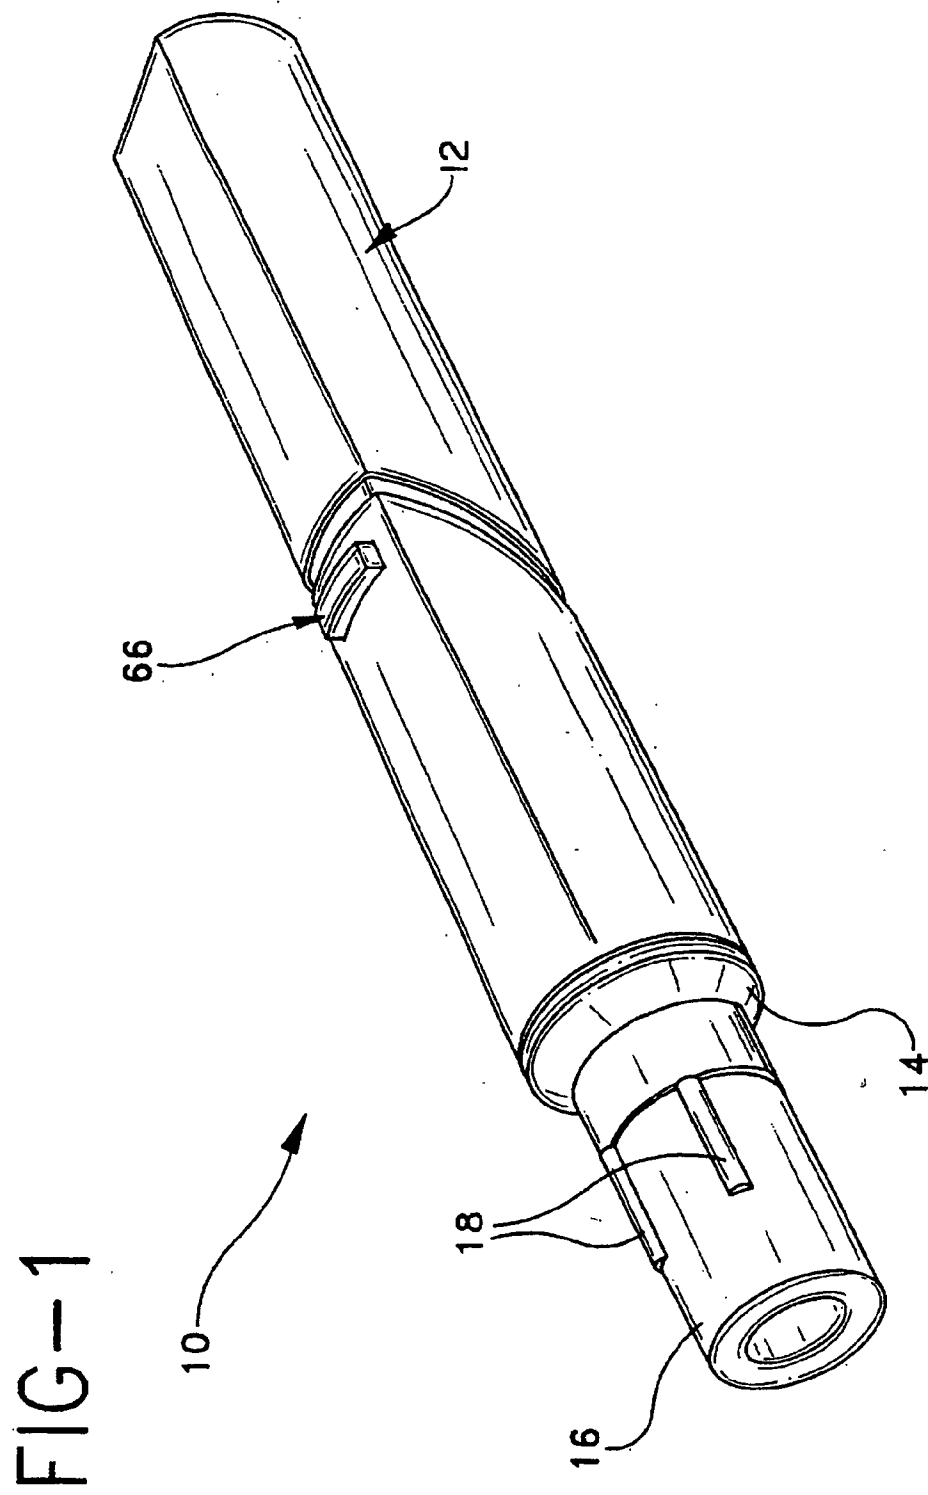

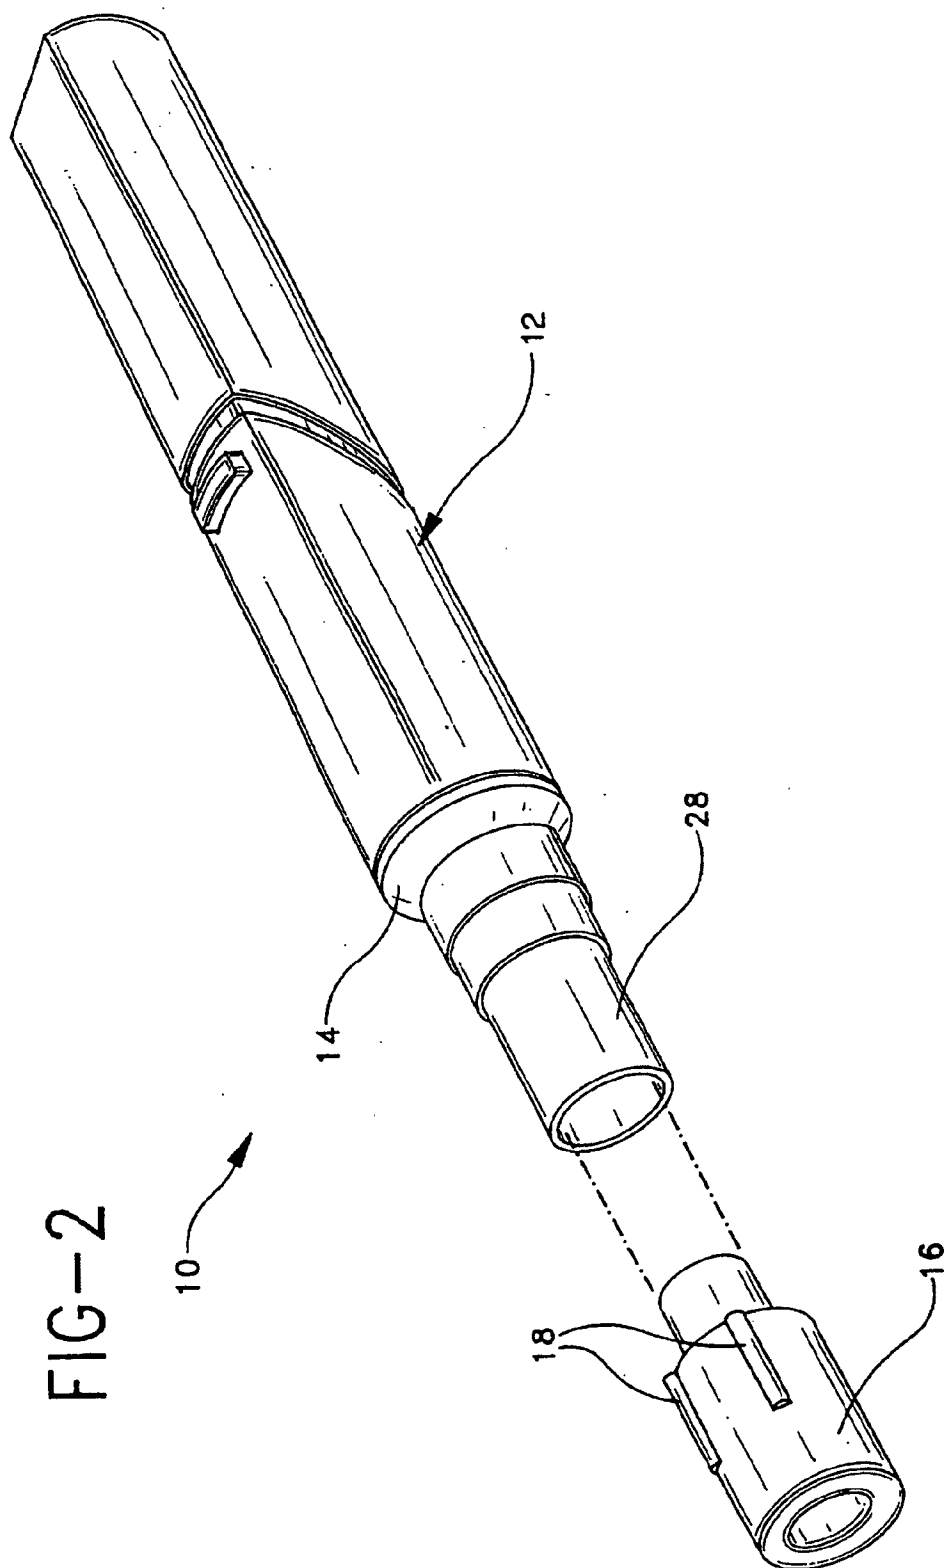

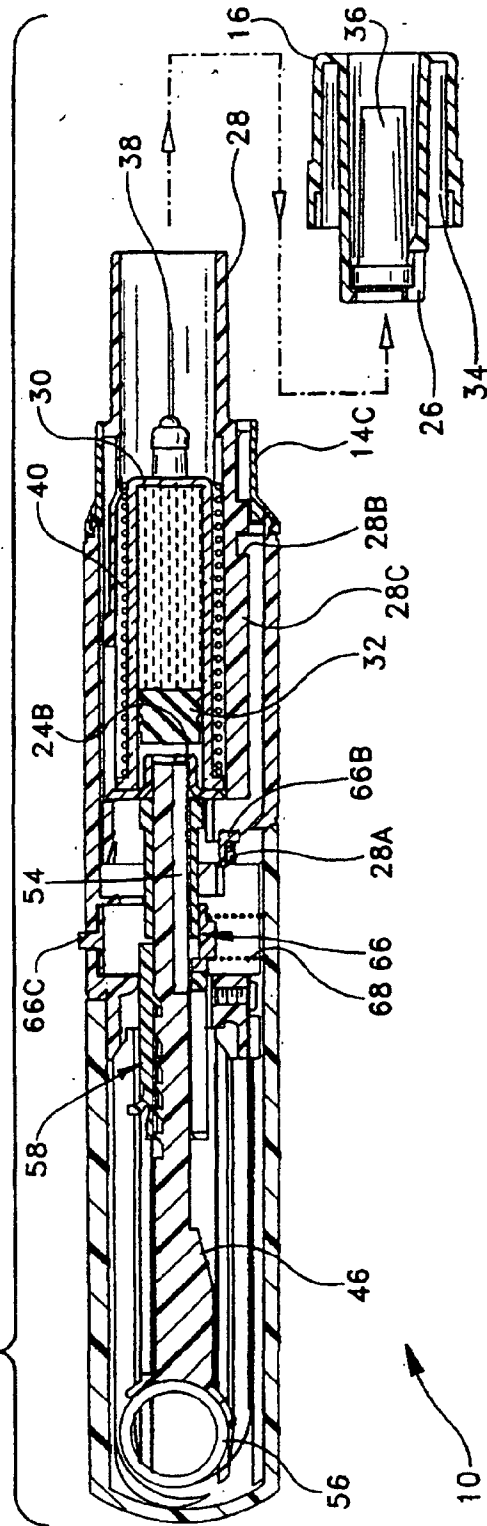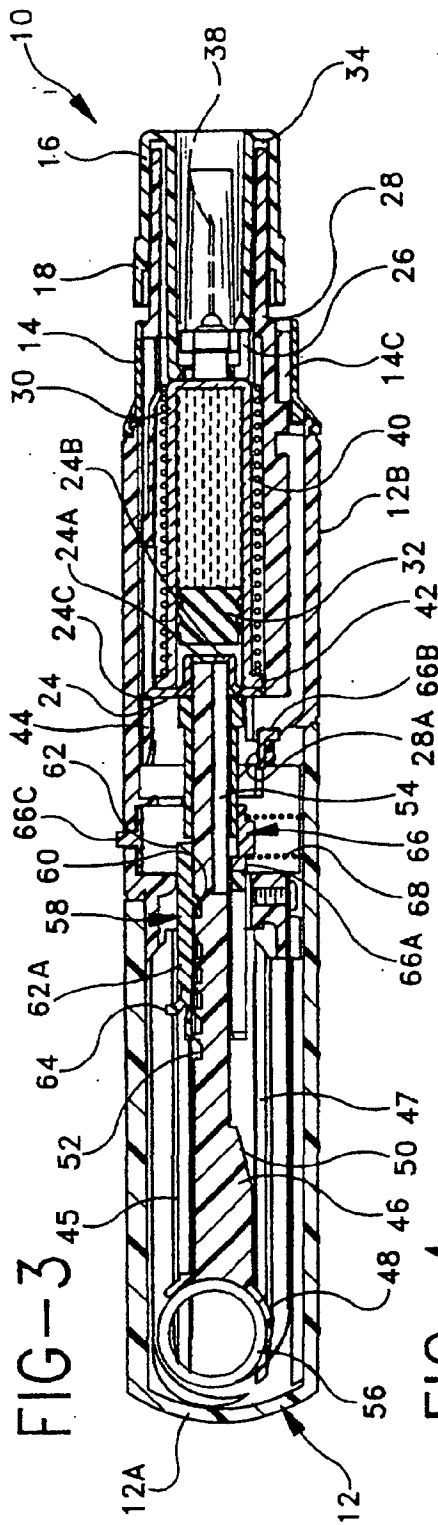

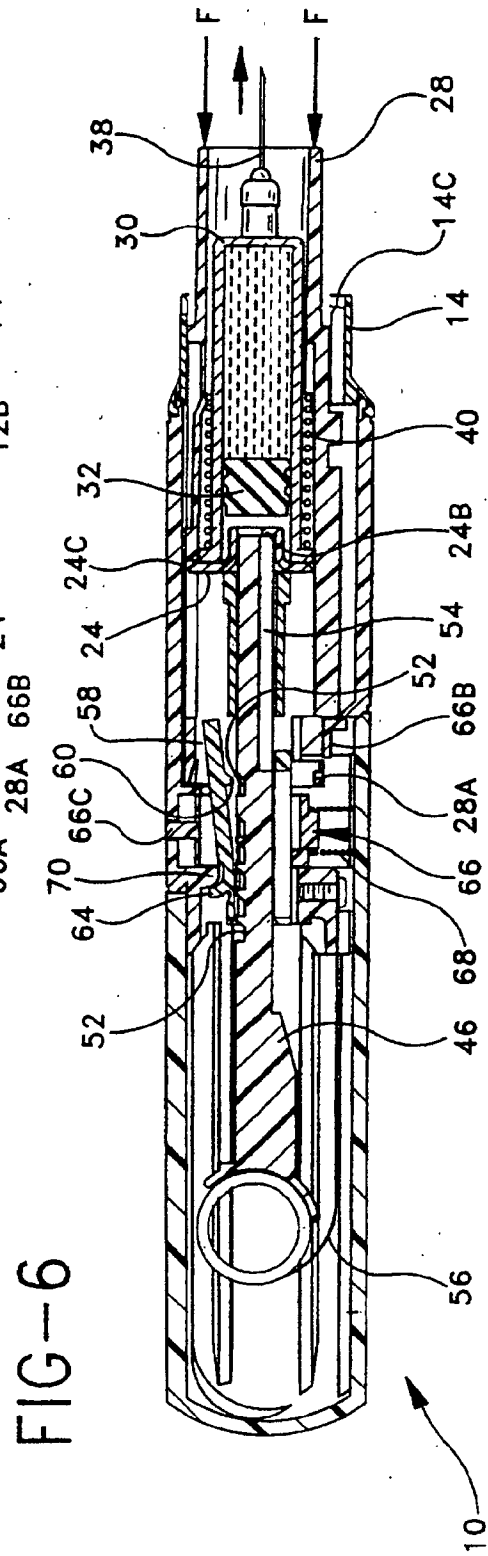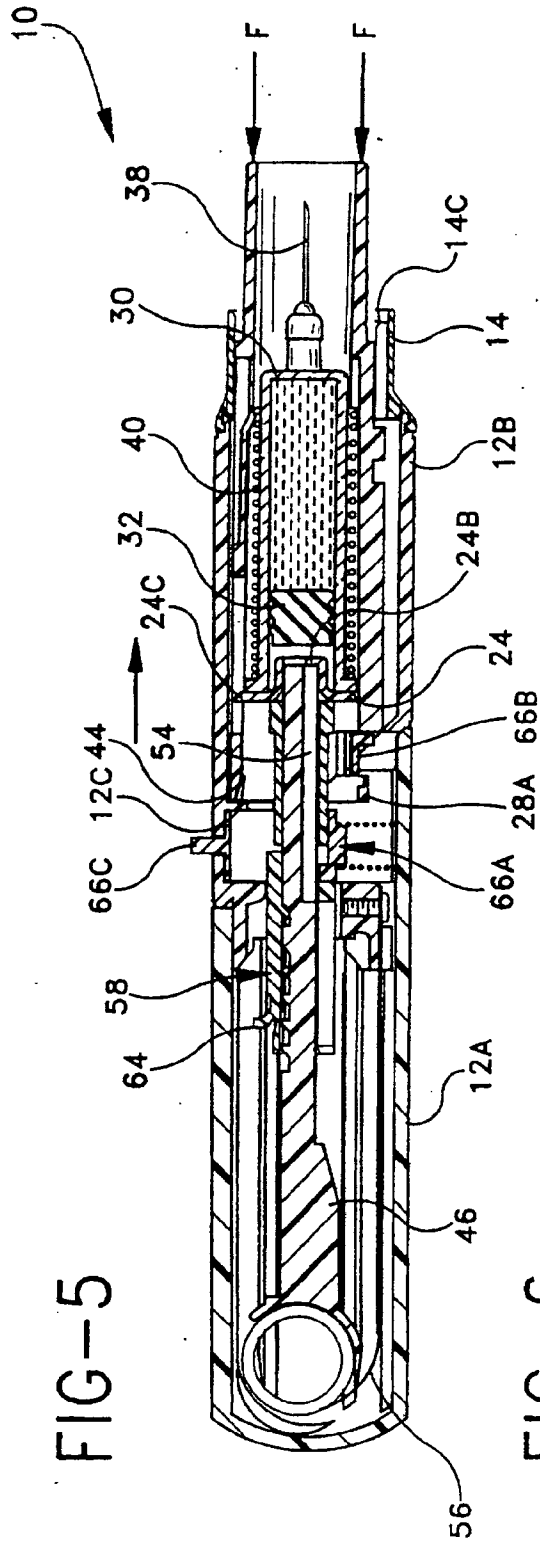

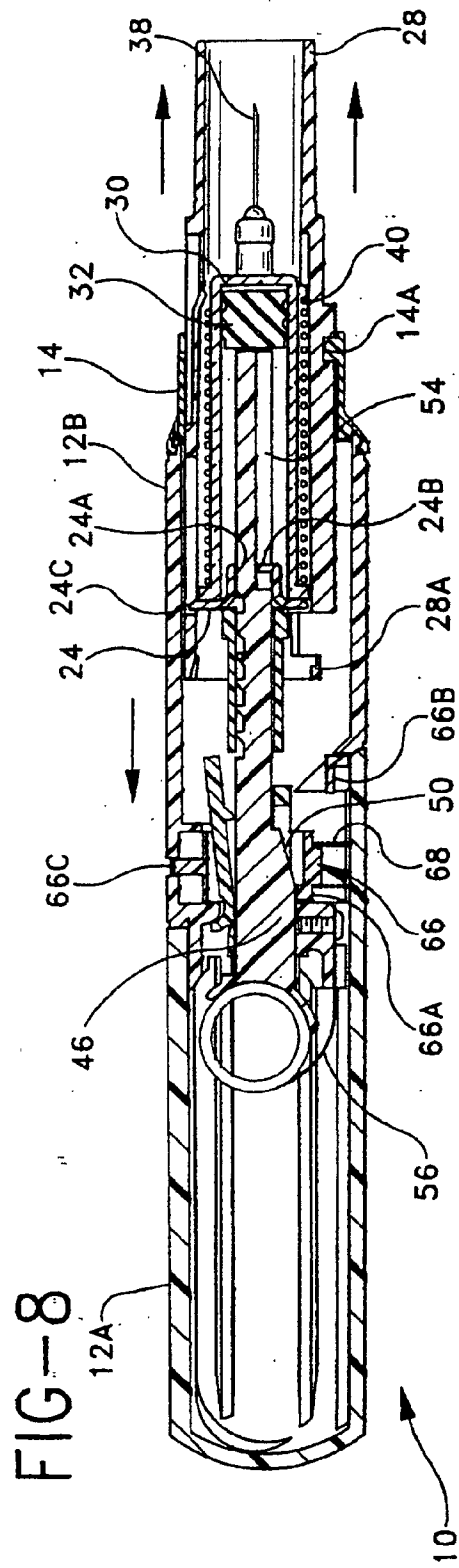
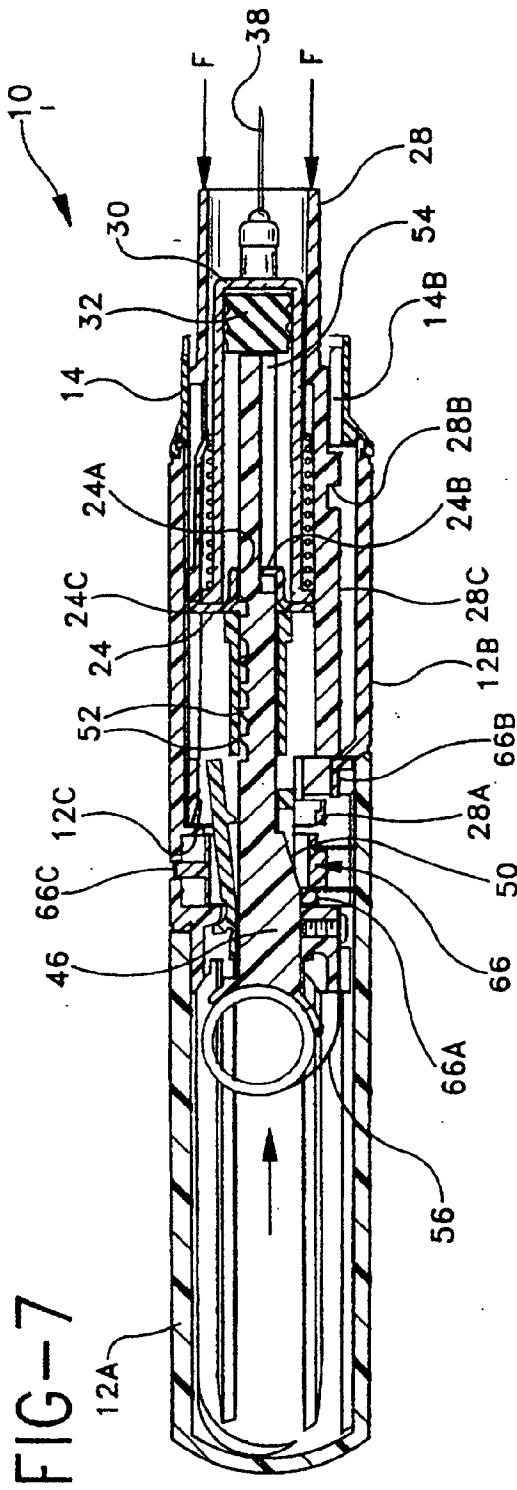
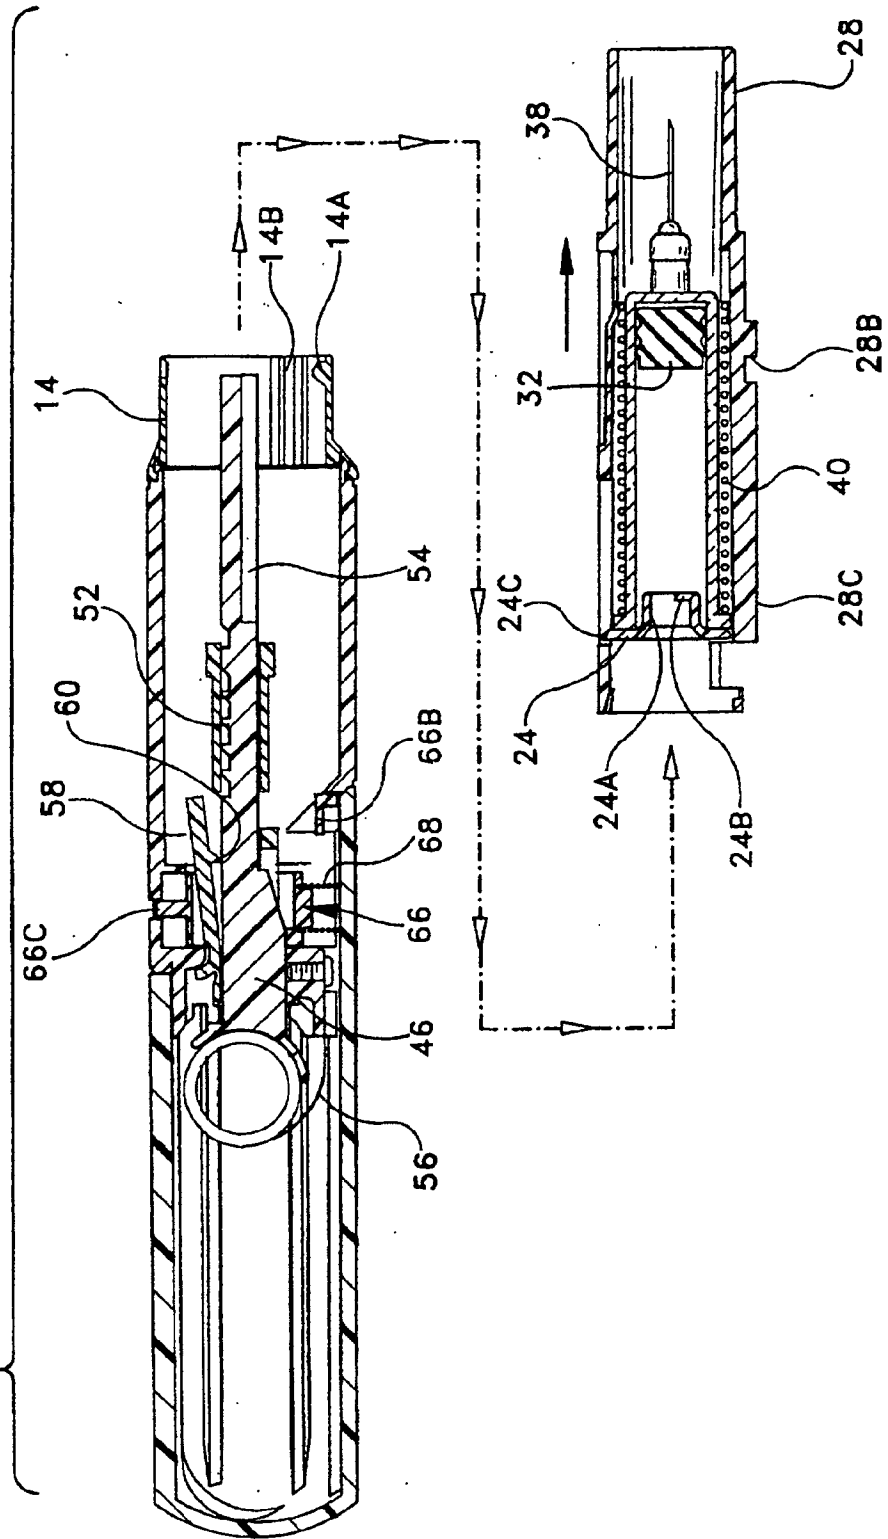
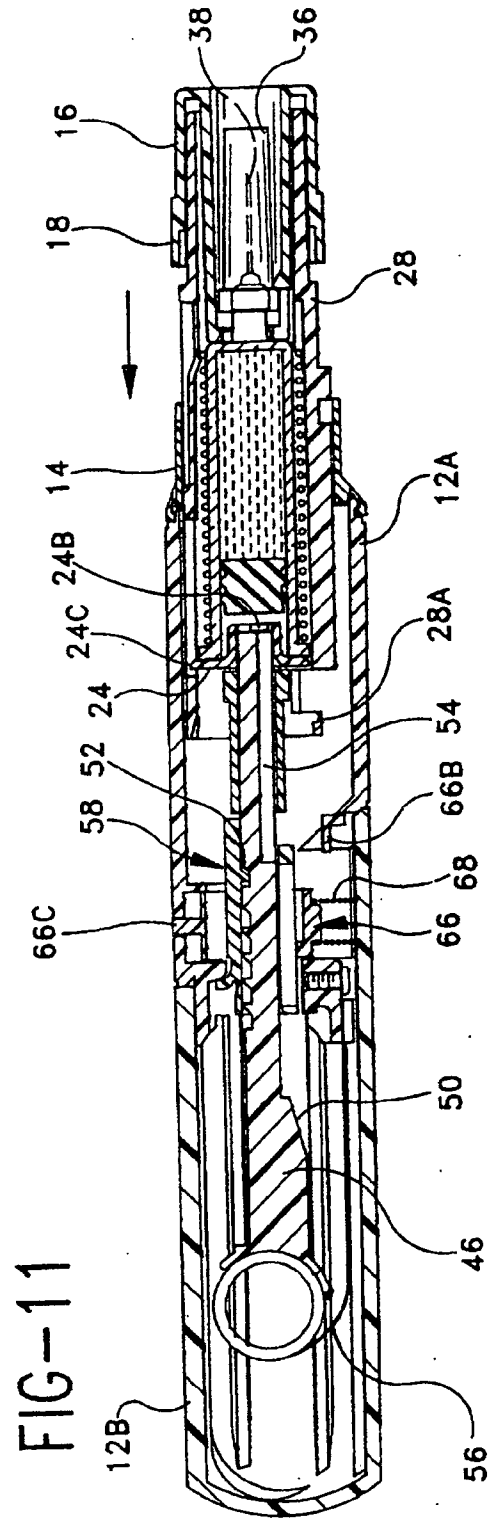
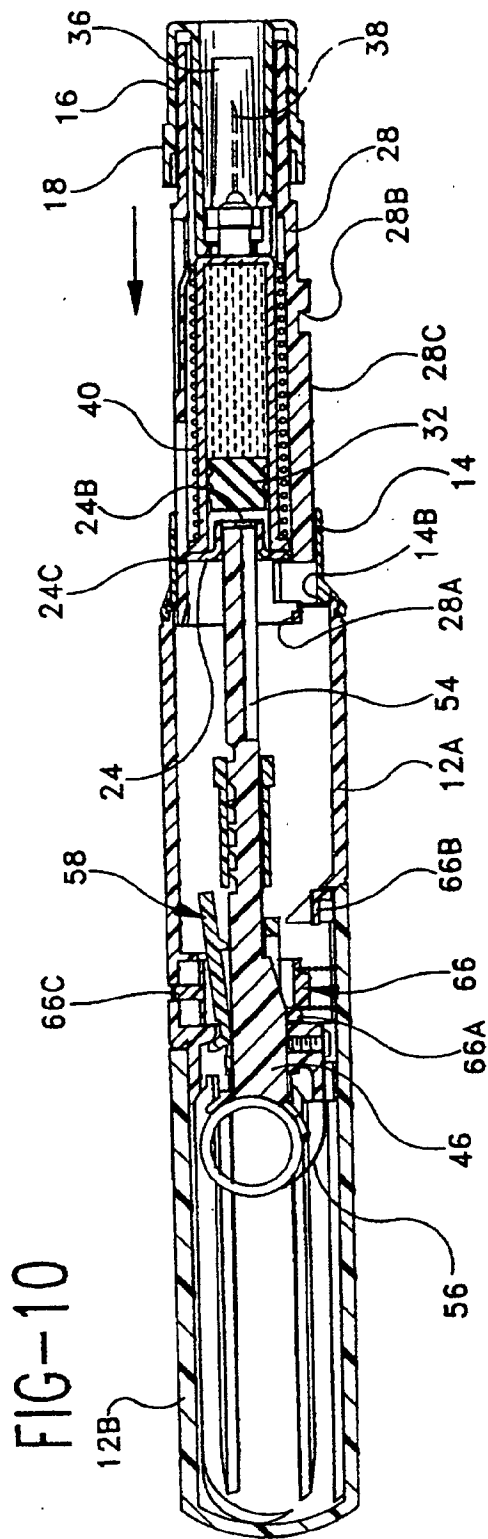


FIG--9





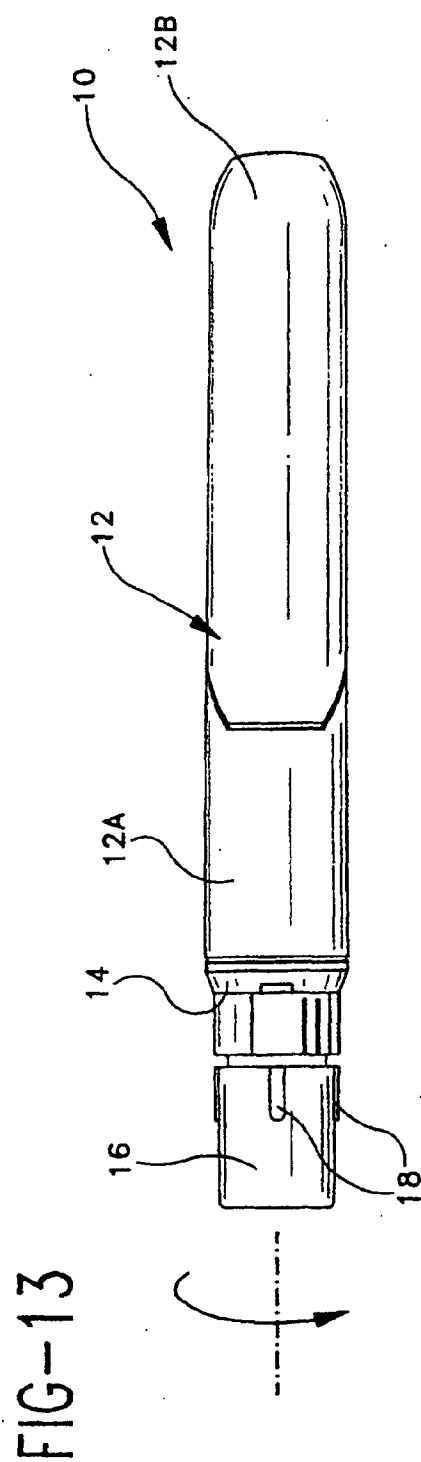
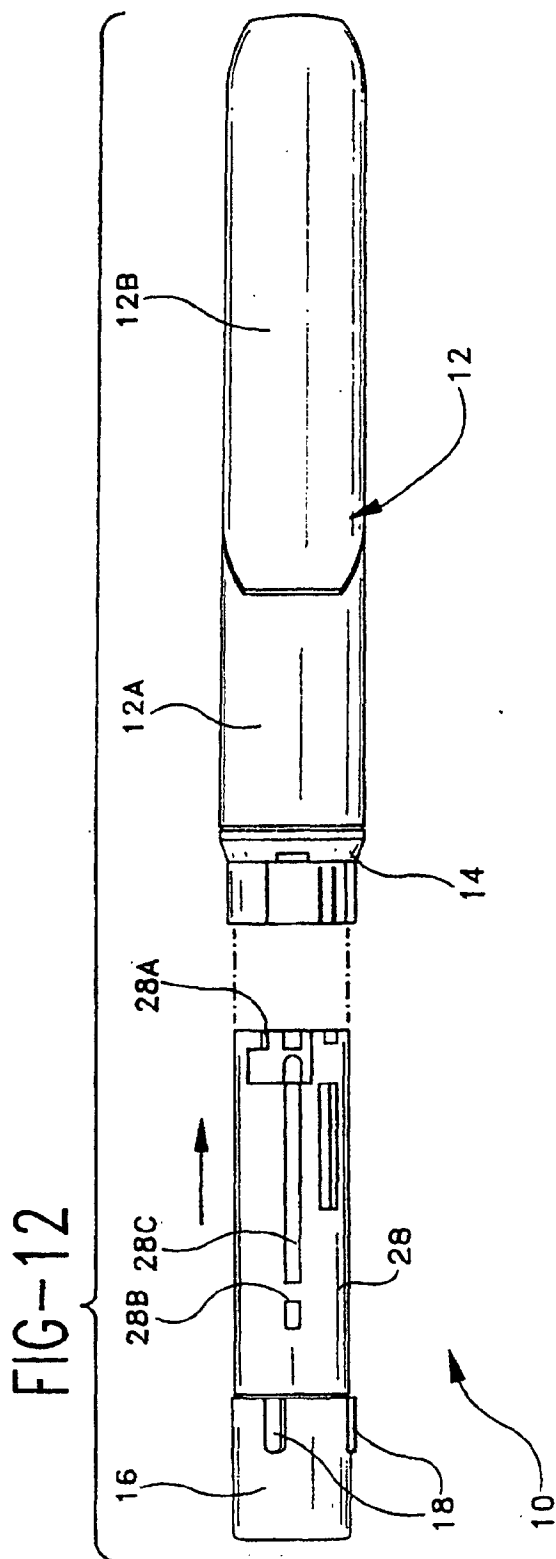


FIG-15

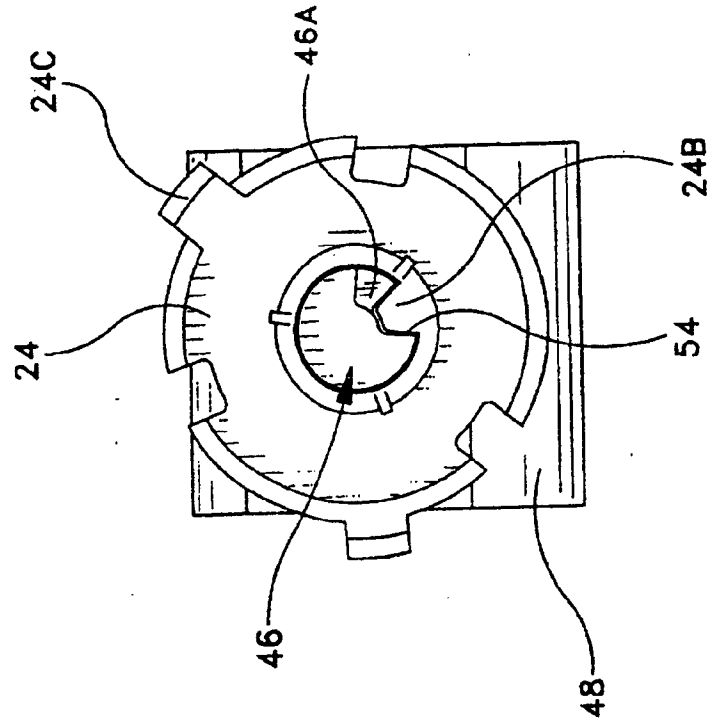


FIG-14

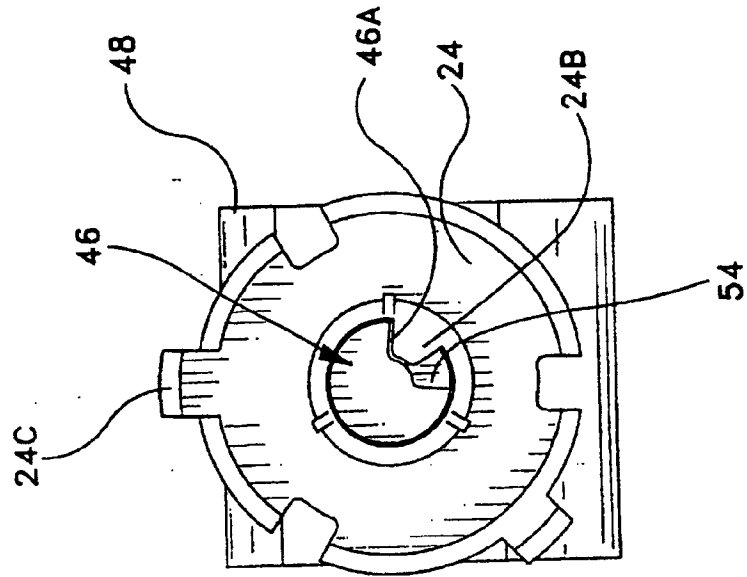


FIG-17

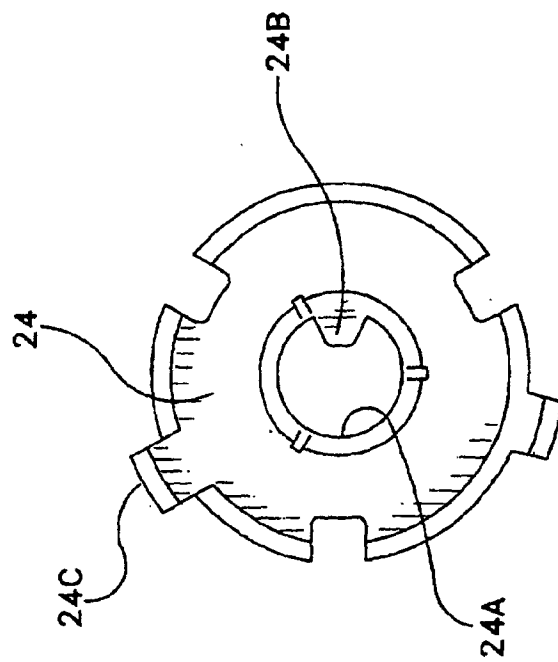


FIG-16

